



MODEL 65 PERCENT OXYGEN PROBE



Operator Manual

MODEL 65 OPERATOR MANUAL

Special Message from Advanced Micro Instruments® (AMI):

Thank you for purchasing this **MODEL 65** for your Percent Oxygen measurement needs. This Percent Oxygen Probe is designed for OEM applications, requiring measurement of percent oxygen levels in inert gases. You will find that it delivers the highest levels of performance and reliability and can be mounted virtually anywhere in a NON-FLAMMABLE environment.

Note: Read this manual carefully prior to installation.

If you have any questions, contact AMI at 714.848.5533 or www.amio2.com.

TABLE OF CONTENTS

MODEL 65 Overview _____	2
Method of Measurement _____	3
Safety, Warnings & Cautions _____	3
Oxygen Probe Installation _____	4
Oxygen Probe Calibration _____	6
Sensor Replacement _____	7
Troubleshooting / Service _____	7
Oxygen Probe Accessories _____	8
Specifications _____	9
AMI Warranty & Support _____	10
Limited Warranty/Disclaimer _____	10
Limitation of Liability _____	10
Limitation of Remedies _____	10

ANALYZER OVERVIEW



METHOD OF MEASUREMENT: ZIRCONIUM OXIDE SENSORS

The **MODEL 65** utilizes zirconium oxide sensors, which provides reliable, accurate percent oxygen measurements for a general purpose environment.

- These sensors have a 10-year product life. This eliminates the need to replace sensors every 6 months and the need to perform monthly calibrations, which drastically lowers maintenance costs.



SAFETY, WARNINGS & CAUTIONS



Make sure no hazardous gas is present in the area before and during installation.

Violation of the National Electrical Code requirements (especially Article 500 that deals with hazardous areas) may cause a fire or explosion with the potential for serious injury or loss of life.



Do not mount the unit in a hazardous area. If explosive gases are present, they can be ignited by the zirconium oxide sensor.


OXYGEN PROBE INSTALLATION

Part I: Mounting the Analyzer

Key Points:

- The Percent Oxygen Probe is designed to be mounted in a general-purpose area. Do not install it in a hazardous area containing flammable gases.

1. Mount the Percent Oxygen Probe in the location, where the measurements will be taken.
2. The included Mounting Bracket accessory, can be used to assist in the installation of the Probe.

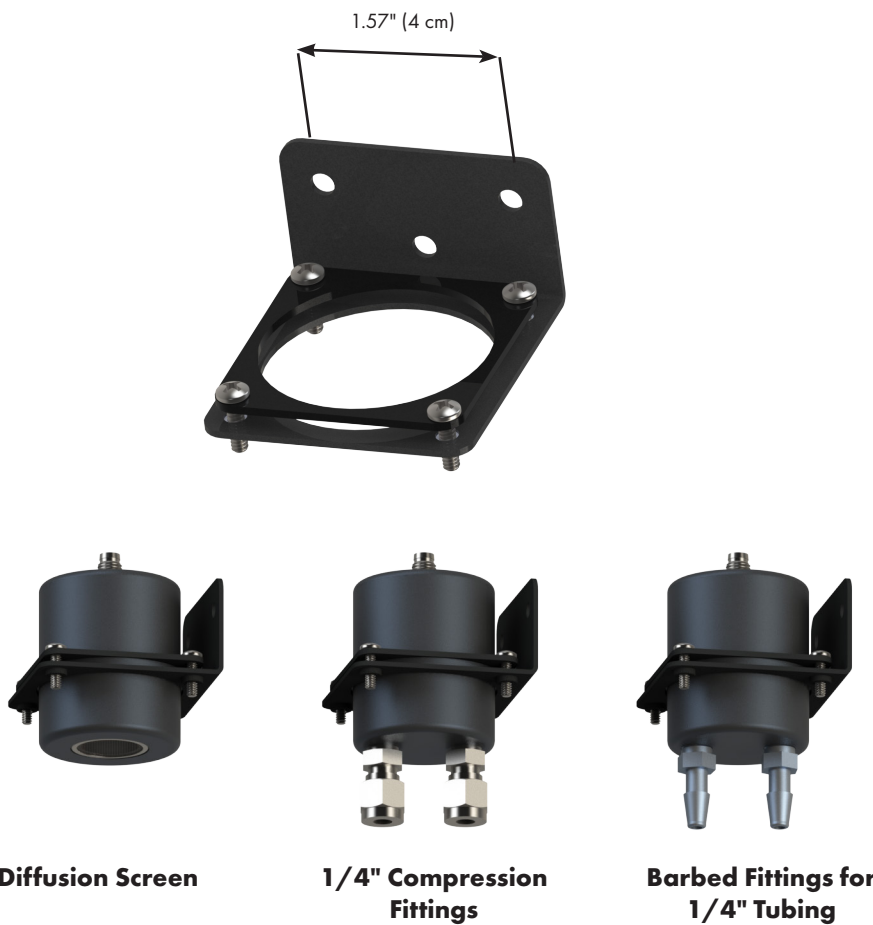

Pictured: The Oxygen Probe with the 3 different gas connection options installed with the Mounting Bracket.



CAUTION:

The **MODEL 65** is designed for operation between 14°F and 122°F (-10°C and 50°C).

Part III: Gas Connections

Key Points:

- The Percent Oxygen Probe has 3 gas connection options, which must be specified at time of purchase.



Diffusion Screen



1/4" Compression Fittings



**Barbed Fittings for
1/4" Tubing**

1. Connect the source of the gas to be measured to the gas connection of the Percent Oxygen Probe.
 2. The Percent Oxygen Probe is now ready to perform measurements.
-

CALIBRATION

Note: The **MODEL 65** Percent Oxygen Probe has already been calibrated at the factory and is ready for use upon arrival. No initial calibration is required from the operator.

SENSOR REPLACEMENT



The MODEL 65 is shipped from our factory with the zirconium oxide sensor already installed inside.

The zirconium oxide sensor has a product life of 10 years.

To replace the sensor near the end of its product life, contact AMI to make arrangements. The sensor can only be replaced inside the MODEL 65 at our factory.

TROUBLESHOOTING/SERVICE

The MODEL 65 has no serviceable parts inside. If you encounter an issue with your unit, contact AMI for support and to obtain a Return Material Authorization (RMA).

ACCESSORIES

The MODEL 65 comes with 2 included accessories.

6-FT CORD



The yellow cord is connected to the MODEL 65 to supply power to the unit.

MOUNTING BRACKET



The Mounting Bracket can be used to assist in the mounting of the Percent Oxygen Probe.

SPECIFICATIONS

PHYSICAL

Dimensions _____ 2.0" L x 2.2" D (51 mm x 56 mm)

Weight _____ < 1.0 lbs (0.5 kg)

Installation _____ Integrated as a Standalone Oxygen Sensor

Gas Connections Options _____ Diffusion screen, 1/4" ID tubing for Barbed Fittings
or 1/4" Compression Fittings

TECHNOLOGY

Method of Measurement _____ Zirconium Oxide Sensor (Up to 10-year life expectancy)

PERFORMANCE

Repeatability _____ $\pm 1\%$ of range or $\pm 0.2\%$ of oxygen, whichever is greater

Operational Conditions _____ Pollution degree 2, Installation Category II

OPERATION

Measurement Range & Analog Output _____ 0.0% – 25.0% (0 – 2.5 VDC or 4 – 20 mA),
0.0% – 50.0% (0 – 2.5 VDC or 4 – 20 mA),
or 0.0% – 95.0% (0 – 4.0 VDC or 4 – 20 mA)

Operating Temperature Range _____ 14°F to 122°F (-10°C to 50°C)

Gas Pressure _____ 17 psig max

Recommended Flow Rate _____ 0.1 to 5.0 SCFH (0.05 – 2.3 Lpm)

AREA CLASSIFICATION

Area Classification _____ Designed for General Purpose /
NON-FLAMMABLE GAS Environments

ACCESSORIES

Included _____ 6-ft Cable,
Mounting Bracket

POWER

Requirements _____ 12 – 24 VDC, 500 mA max

AMI WARRANTY & SUPPORT

LIMITED WARRANTY/DISCLAIMER

The warranty period is **TWO YEARS** for the Analyzer. Any failure of material or workmanship will be repaired free of charge for that specified period from the original purchase (shipping date) of the instrument. AMI will also pay for 1-way ground shipment back to the customer.

The warranty period for the electrochemical oxygen sensor is 6 months.

The warranty period for the electrochemical H₂S sensor is 6 months.

The warranty period for the zirconium oxide sensor is 2 years.

Any indication of abuse or tampering of the instrument will void the warranty.

Receiving the Analyzer

When you receive the instrument, check the package for evidence of damage and if any is found contact the shipper. Although every effort has been made to assure that the Analyzer meets all performance specifications, AMI takes no responsibility for any losses incurred by reason of the failure of this analyzer or associated components. AMI's obligation is expressly limited to the Analyzer itself.

EXCEPT FOR THE FOREGOING LIMITED WARRANTY, AMI MAKES NO WARRANTIES, EXPRESS, IMPLIED OR STATUTORY, AS TO THE NON-INFRINGEMENT OF THIRD-PARTY RIGHTS, MERCHANTABILITY, OR FITNESS FOR A PARTICULAR PURPOSE. IF APPLICABLE LAW REQUIRES ANY WARRANTIES WITH RESPECT TO THE SYSTEM, ALL SUCH WARRANTIES ARE LIMITED IN DURATION TO TWO (2) YEARS FROM THE DATE OF DELIVERY.

LIMITATION OF LIABILITY

IN NO EVENT WILL AMI BE LIABLE TO YOU FOR ANY SPECIAL DAMAGES, INCLUDING ANY LOST PROFITS, LOST SAVINGS, OR OTHER INCIDENTAL OR CONSEQUENTIAL DAMAGES, EVEN IF THE COMPANY HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES, OR FOR ANY CLAIM BY ANY OTHER PARTY.

LIMITATION OF REMEDIES

AMI's entire liability and your exclusive remedy under the Limited Warranty (see above) shall be the replacement of any Analyzer that is returned to the Company and does not meet the Company's Limited Warranty.

FACTORY SERVICE AND SUPPORT

AMI offers calibration and repair services for their analyzers. To return an analyzer to the factory for repair or calibration, please complete a Return Merchandise Authorization (RMA) Request Form at www.amio2.com/request-rma. After your form has been received and reviewed, an AMI representative will contact you by email or phone with RMA number and instructions on how to ship the unit to the AMI factory.

If you have questions about your product, please contact the AMI factory at +1.714.848.5533 or complete the online Service & Support form at www.amio2.com/quote/support.



HIGH PERFORMANCE

RELIABILITY

INTUITIVE DESIGN

www.amio2.com

Tel 714.848.5533
Email sales@amio2.com

OM-300-006 Rev H
2026.01

© Advanced Micro Instruments, Inc.

ADDRESS:

Advanced Micro Instruments, Inc.
15501 Red Hill Avenue, Suite 100
Tustin, CA 92780 USA

